

[View on rigaku.com](https://www.rigaku.com)

BATT1017 - XRD Measurement during Charge/Discharge Using All-Solid-State Batteries

Introduction

All-solid-state Na ion batteries are next-generation batteries that are expected to be less expensive than Li ion batteries and have faster charge/discharge performance. When operating all-solid-state batteries, it is necessary to continue applying pressure to make it easier for the ions to move within the solid. With this measurement, using cells that can be charged/discharged while applying pressure to an all-solid-state battery, the behavior of an all-solid-state Na ion battery was verified.

Phase transition analysis

- **Analysis:** Whole battery
- **Analysis method:** Operando measurement
- **Use:** Improving battery performance
- **Analyzed materials:** All-solid-state Na ion batteries (Cathode TiS_2 , solid-state electrolyte Na_3PS_4 , anodes)
- **Accessory:** All-solid-state battery cells

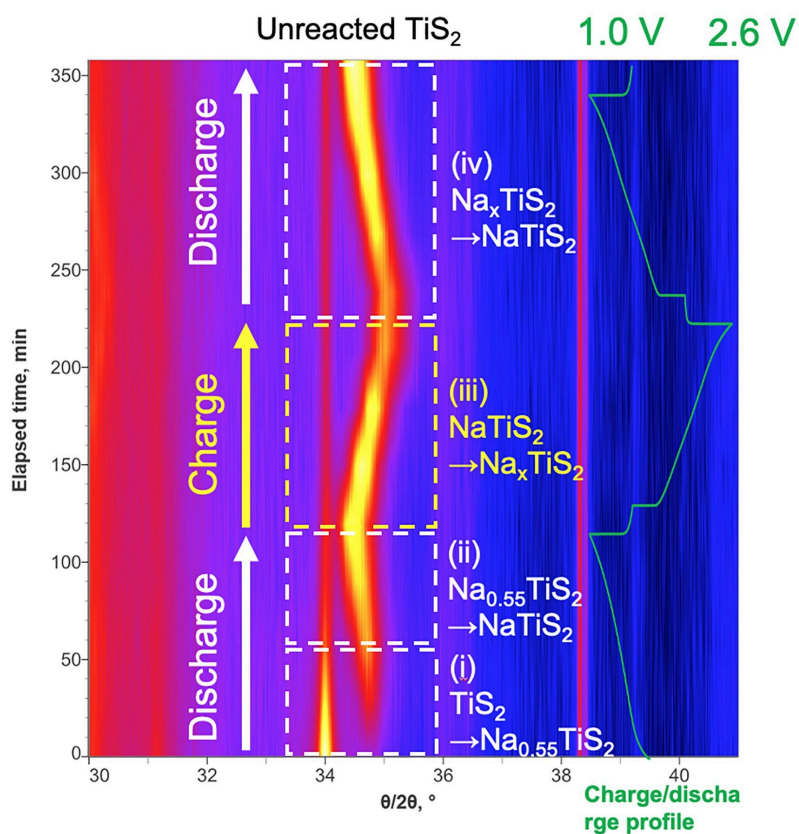


Figure 1: Elapsed time vs 2θ and charge/discharge profile (inside image)




Figure 2: Representation of solid-state battery pellet and pressure conditions

Cathode TiS_2 exhibited the following changes during charging/discharging.

Phase transition from $\text{TiS}_2 \rightarrow \text{Na}_{0.55}\text{TiS}_2$

- (i) Change in lattice constant from $\text{Na}_{0.55}\text{TiS}_2 \rightarrow \text{NaTiS}_2$
- (ii) Change in lattice constant from $\text{NaTiS}_2 \rightarrow \text{Na}_x\text{TiS}_2$ ($x < 0.55$)
- (iii) Change in lattice constant from $\text{Na}_x\text{TiS}_2 \rightarrow \text{NaTiS}_2$

(iv) Unreacted TiS_2 was partially present

Conclusion

It is possible to measure changes in the crystal phase and lattice constant during charging/discharging in an all-solid-state battery.

Related products



SmartLab

Advanced state-of-the-art high-resolution XRD system powered by Guidance expert system software